

**THERMOMETERS APPROVED TO MEASURE THE TEMPERATURE OF
SIMULATOR SOLUTIONS**

I, Barry K. Logan, certify under penalty of perjury under the laws of the State of Washington that the following is true and correct:

I am the State Toxicologist authorized under RCW 46.61.506 to approve methods for breath alcohol testing within the State of Washington.

The following instruments are approved for the quantitative measurement of alcohol in a person's breath:


- A) The DataMaster
- B) The DataMaster CDM

These are the only two instruments utilized in the Washington State Patrol's breath-testing program.

A Guth Model 34C or Guth 2100 wet bath simulator device is attached to every DataMaster and DataMaster CDM. Each Guth Model 34 C simulator employs a mercury in glass thermometer with a scale graduated in tenths of a degree measuring a range between 33.5 and 34.5 degrees centigrade. Each Guth 2100 wet bath simulator employs a digital thermometer.

Persons who received their certification to conduct breath tests as described in WAC 448-16 have been trained and are certified to perform tests on the DataMaster, the DataMaster CDM, and portable breath test devices as described in WAC 448-15.

EXECUTED this 25th day of March, 2005, at Seattle, Washington

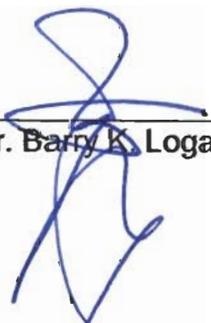

Dr. Barry K. Logan, State Toxicologist